


Bioavailability (%)

2/4

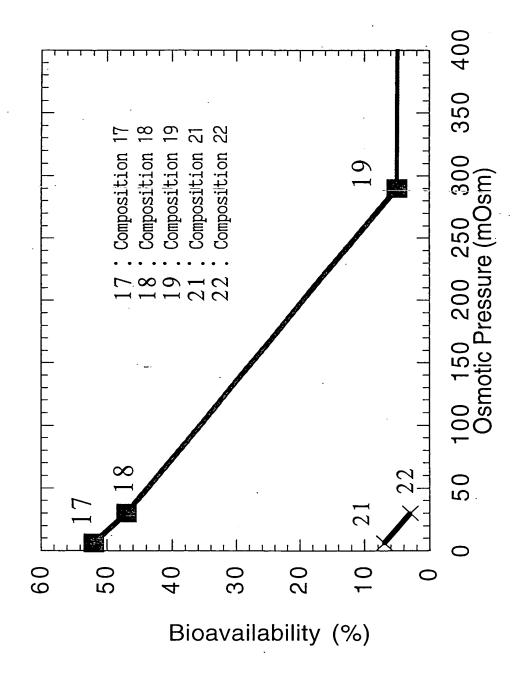



gring filter for the hole film inter copy can be taken to the copy of the copy

•

-

The state with the state of the

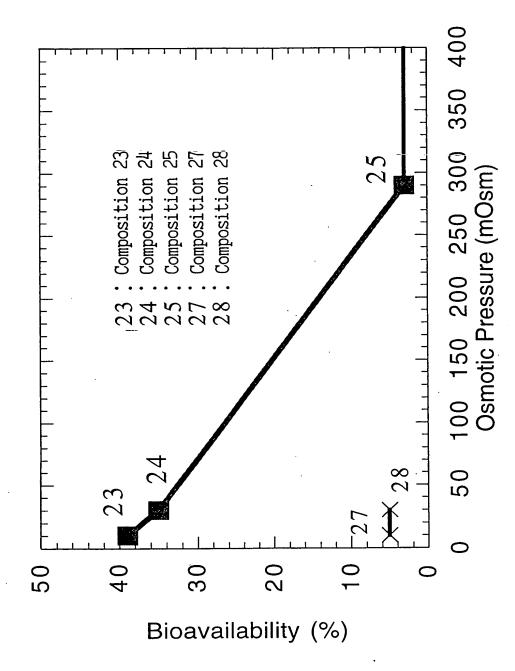




4/4

Fig.4

(A)

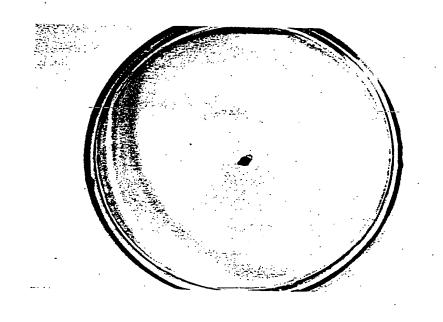

(B)

